

Other AlphaScreen™ Products

Contact us

Beads*

- Streptavidin-coated Donor beads
- Unconjugated Donor beads
- Unconjugated Acceptor beads
- Conjugation kit**

Fusion Tag Detection Kits***

- GST (Glutathione-S-Transferase) detection kit
- DIG (Digoxin/Digoxigenin) detection kit
- FITC (Fluorescein) detection kit
- HIS₆ (6-Histidine) detection kit
- Histidine (Nickel chelate) detection kit
- c-myc detection kit
- HA (Hemagglutinin) detection kit
- FLAG™ (M2) detection kit

IgG Detection Kits***

- Goat IgG detection kit
- Human IgG detection kit
- Mouse IgG detection kit
- Rabbit IgG detection kit
- IgG (Protein A) detection kit

GPCR Functional Assay Kits

- cAMP assay kit****
- IP₃ assay supplement***** (Requires GST detection kit)

Phosphotyrosine Assay Kits***

- Phosphotyrosine (PY20) assay kit
- Phosphotyrosine (PT66) assay kit
- Phosphotyrosine (P-Tyr-100) assay kit

* Available in 1, 5 and 50 mg quantities. 1 mg translates into 2,000 assay points based on a 25 µL reaction volume and final bead concentration of 20 µg/mL.

** 2 mg ea. streptavidin-coated Donor beads / unconjugated Acceptor beads.

*** Available in 500, 10,000 and 50,000 assay point quantities based on a 25 µL reaction volume and final bead concentration of 20 µg/mL.

**** Available in 500, 10,000 and 50,000 assay point quantities based on a 25 µL reaction volume and final donor and acceptor bead concentration of 20 µg/mL and 15 µg/mL, respectively.

***** Available in 500 and 10,000 assay point quantities based on a 50 µL reaction volume and final bead concentration of 10 µg/mL.

Microplates and Microplate Analyzers

Fusion™-α and **AlphaQuest®-HTS** microplate analyzers and **Optiplate™ microplates** are optimized to measure AlphaScreen signal and are available from Packard BioScience Company.

For more information please contact your local Packard BioScience office or visit our website at

www.packardbioscience.com

For technical assistance please contact:

BioSignal Packard Inc.

1744 William Suite 600,
Montréal (Québec), Canada H3J 1R4
<http://www.biosignalspackard.com>
Customer Support: Tel.: 514-937-1010
Toll Free: 1-800-293-4501
Fax: 514-937-0777
E-mail: alphascreen@packardbioscience.com

To place an order and for all other assistance please contact:

Packard BioScience Company (Head Office)

800 Research Parkway
Meriden, CT 06450 U.S.A.
Tel.: 203-639-2598
Toll Free: 1-800-323-1891
Customer Support: 1-800-445-7426
Fax: 203-639-2172
Web site: <http://www.packardbioscience.com>
E-mail: webmaster@packardbioscience.com

Packard BioScience International Offices:

Australia +(61)-3-95434266;
Austria +(43)-1-2702504;
Belgium +(32)-2-4818530;
Canada (Main Office) +(1)-905-673-8028;
Central Europe +(43)-2-23037000;
Denmark +(45)-43-909023;
France +(33)-1-46862775;
Germany +(49) 6103 385151;
Italy +(39)-02-33910796;
Japan +(81)-3-38665850;
Netherlands +(31)-50-5445900;
Pacific Rim +(852) 2620-1881;
Russia +(7095)-4296577;
Switzerland +(41)-1-4816944;
United Kingdom +(44)-118-9844981

For all international representatives, contact the Packard BioScience U.S.A. office.

6760606C PI Rev.: A 01/2002 © 2001

AlphaScreen™, AlphaQuest™, Fusion™, OptiPlate™ and TopSeal™ are trademarks of Packard BioScience Company.

Milli-Q® is a registered trademark of Millipore Corporation.

LIMITED WARRANTY BioSignal Packard Inc. warrants that, at the time of shipment, the products sold by it are free from defects in material and workmanship and conform to specifications that accompany the product. BioSignal Packard Inc. makes no other warranty, express or implied with respect to the products, including any warranty of merchantability or fitness for any particular purpose. Notification of any breach of warranty must be made within 30 days of receipt unless provided in writing by BioSignal Packard Inc. No claim shall be honoured if the customer fails to notify BioSignal Packard Inc. within the period specified. The sole and exclusive remedy of the customer for any liability of BioSignal Packard Inc. of any kind including liability based upon warranty (express or implied whether contained herein or elsewhere), strict liability contract or otherwise is limited to the replacement of the goods or the refunds of the invoice price of goods. BioSignal Packard Inc. shall not in any case be liable for special, incidental or consequential damages of any kind.

BioSignal Packard Inc.

1744 William Suite 600, Montréal (Québec), Canada H3J 1R4
<http://www.biosignalspackard.com>
Tel.: (514) 937 1010 - in US and Canada (800) 293 4501
Fax. (514) 937 0777

AlphaScreen™ Mouse IgG (mIgG) Detection Kit

Product Information & Titration Curve Protocol



Product Information

AlphaScreen™ Mouse IgG (mIgG) Detection Kit

Catalog No.: **6760606C**
Kit size: **500 assay points***

* The number of assay points is based on a 25 μ L reaction volume and a final bead concentration of 20 μ g/mL.

Kit Components

Anti-mouse IgG (mIgG) Acceptor Beads

1 tube containing 50 μ L anti-mIgG Acceptor beads at 5 mg/mL in 1x PBS, pH 7.2.

Streptavidin Donor Beads

1 tube containing 50 μ L streptavidin Donor beads at 5 mg/mL in 1x PBS, pH 7.2.

Biotinylated-mouse-IgG

1 tube containing 50 μ L biotinylated-mIgG at 50 nM in 1x PBS, 0.1% BSA, pH 7.2.

10x Buffer

1 tube containing 1.5 mL 10x PBS, pH 7.2.

Note: 0.05% Proclin-300 is added as a preservative to all components.

Product QC/QA

Donor and Acceptor beads are controlled to meet chemical composition, dextran loading and conjugation requirements.

AlphaScreen lot-to-lot consistency is confirmed by a competition and titration assay to meet defined specifications under standard conditions.

Titration Curve Protocol

Note: This protocol provides a means to verify kit performance and is not representative of an assay. Sufficient biotinylated-mouse-IgG and 10x buffer is provided to perform 3 titration curves in triplicate as described. To perform an actual assay with the AlphaScreen Mouse-IgG (mIgG) Detection Kit, please refer to the appropriate application notes and protocol books.

Materials & preparation:

1x Buffer

Add 500 μ L 10x buffer to 4.5 mL Milli-Q® H₂O (or equivalent). Add 5 mg BSA (0.1% final concentration) and adjust pH to 7.2.

Note: Before use, warm 10x buffer to room temperature and ensure that any precipitated salt is redissolved.

Anti-mouse IgG (mIgG) Acceptor beads (Provided)


Add 4 μ L anti-mouse IgG (mIgG) Acceptor beads to 196 μ L 1x buffer.

Streptavidin Donor beads (Provided)

Add 4 μ L streptavidin Donor beads to 196 μ L 1x buffer.

Biotinylated-mouse-IgG (Provided)

Starting from the 50 nM provided, prepare a 1/2 log dilution series (5 nM to 0.5 pM) in 1x buffer as illustrated. Include a buffer only control.

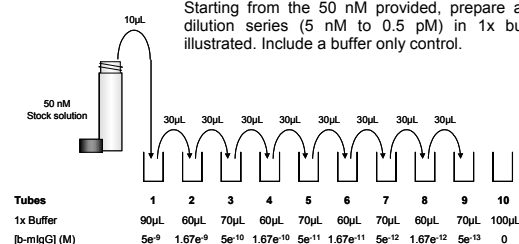


Method:

To a 384-well white opaque Optiplate™-384 NEW* (Packard BioScience part number 6007290):

1. Add 15 μ L biotinylated-mouse-IgG dilutions (tubes 1 through 10).
2. Add 5 μ L anti-mouse IgG Acceptor bead.
3. Add 5 μ L streptavidin Donor beads.

Incubate** in the dark*** at room temperature for at least 60 minutes and analyze on either the AlphaQuest™-HTS or Fusion™- α microplate analyzer.

Result:



The above graph illustrates a typical biotinylated-mouse-IgG titration curve performed as described (25 μ L final volume in a 384-well microplate) at room temperature (22-23°C) and 1 hour incubation. Total signal will vary with ambient temperature and incubation time. Signal is stable with an overnight incubation. For consistent results, the same incubation times and temperature should be used for each plate.

Final concentrations of reagents in the assay are 20 μ g/mL Donor beads, 20 μ g/mL Acceptor beads, and biotinylated-mouse-IgG at 3 nM, 1 nM, 0.3 nM, 0.1 nM, 0.03 nM, 0.01 nM, 3 pM, 1 pM, 0.3 pM and 0 M.

Precautions

1. AlphaScreen beads are light sensitive.

- Take care to not expose beads to bright light. Beads are best handled under subdued or green filtered light conditions.
- Incubation steps involving the beads should be performed in the dark. Plates can be covered by another microplate to minimize the effect of light.

2. Storage.

- Beads should be stored in the dark at 4°C.
- To ensure product longevity, unused AlphaScreen reagents should be stored in the original packaging, at the original concentration and at the recommended temperature.
- Do not store reagents containing BSA for more than 1 day at 4°C.

3. Interfering compounds.

- For information on potential interfering compounds please refer to application note ASC-012.

* It is recommended that the following steps be performed in triplicate.

** Plates can be covered with TopSeal™ (Packard BioScience part number 6005185) adhesive sealing film to reduce evaporation during incubation.

*** Plates can be covered by another microplate.